



**Designation: A609/A609M – 12 (Reapproved 2023)**

## **Standard Practice for Castings, Carbon, Low-Alloy, and Martensitic Stainless Steel, Ultrasonic Examination Thereof<sup>1</sup>**

This standard is issued under the fixed designation A609/A609M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the U.S. Department of Defense.*

### **1. Scope**

1.1 This practice<sup>2</sup> covers the standards and procedures for the pulse-echo ultrasonic examination of heat-treated carbon, low-alloy, and martensitic stainless steel castings.

1.2 This practice is to be used whenever the inquiry, contract, order, or specification states that castings are to be subjected to ultrasonic examination in accordance with Practice A609/A609M.

1.3 This practice contains two procedures. Procedure A is the original A609/A609M practice and requires calibration using a series of test blocks containing flat-bottomed holes. It also provides supplementary requirements for angle beam testing. Procedure B requires calibration using a back wall reflection from a series of solid calibration blocks.

NOTE 1—Ultrasonic examination and radiography are not directly comparable. This examination technique is intended to complement Guide E94/E94M in the detection of discontinuities.

1.4 Supplementary requirements of an optional nature are provided for use at the option of the purchaser. The supplementary requirements shall apply only when specified individually by the purchaser in the purchase order or contract.

1.5 The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in nonconformance with the standard.

1.5.1 Within the text, the SI units are shown in brackets.

1.5.2 This practice is expressed in both inch-pound units and SI units; however, unless the purchase order or contract specifies the applicable M-specification designation (SI units), the inch-pound units shall apply.

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee A01 on Steel, Stainless Steel and Related Alloys and is the direct responsibility of Subcommittee A01.18 on Castings.

Current edition approved Nov. 1, 2023. Published November 2023. Originally approved in 1970. Last previous edition approved in 2018 as A609/A609M – 12 (2018). DOI: 10.1520/A0609\_A0609M-12R23.

<sup>2</sup> For ASME Boiler and Pressure Vessel Code applications, see related Specification SA-609 of Section II of that Code.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

### **2. Referenced Documents**

#### **2.1 ASTM Standards:<sup>3</sup>**

A217/A217M Specification for Steel Castings, Martensitic Stainless and Alloy, for Pressure-Containing Parts, Suitable for High-Temperature Service

E94/E94M Guide for Radiographic Examination Using Industrial Radiographic Film

E317 Practice for Evaluating Performance Characteristics of Ultrasonic Pulse-Echo Testing Instruments and Systems without the Use of Electronic Measurement Instruments

#### **2.2 Other Document:<sup>4</sup>**

SNT-TC-1A Recommended Practice for Nondestructive Testing Personnel Qualification and Certification

### **3. Ordering Information**

3.1 The inquiry and order should specify which procedure is to be used. If a procedure is not specified, Procedure A shall be used.

3.2 The purchaser shall furnish the following information:

3.2.1 Quality levels for the entire casting or portions thereof,

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>4</sup> Available from American Society for Nondestructive Testing (ASNT), P.O. Box 28518, 1711 Arlingate Ln., Columbus, OH 43228-0518, <http://www.asnt.org>.

3.2.2 Sections of castings requiring longitudinal beam examination,

3.2.3 Sections of castings requiring dual element examination,

3.2.4 Sections of castings requiring supplementary examination, using the angle beam procedure described in Supplementary Requirement S1 in order to achieve more complete examination, and

3.2.5 Any requirements additional to the provisions of this practice.

## PROCEDURE A – FLAT-BOTTOMED HOLE CALIBRATION PROCEDURE

### 4. Apparatus

#### 4.1 Electronic Apparatus:

4.1.1 An ultrasonic, pulsed, reflection type of instrument that is capable of generating, receiving, and amplifying frequencies of at least 0.5 to 5 MHz.

4.1.2 The ultrasonic instrument shall provide linear presentation (within  $\pm 5\%$ ) for at least 75 % of the screen height (sweep line to top of screen). Linearity shall be determined in accordance with Practice E317 or equivalent electronic means.

4.1.3 The electronic apparatus shall contain a signal attenuator or calibrated gain control that shall be accurate over its useful range to  $\pm 10\%$  of the nominal attenuation or gain ratio to allow measurement of signals beyond the linear range of the instrument.

#### 4.2 Search Units:

4.2.1 *Longitudinal Wave*, internally grounded, having a  $\frac{1}{2}$  to 1 in. [13 to 25 mm] diameter or 1 in. [25 mm] square piezo-electric elements. Based on the signals-to-noise ratio of the response pattern of the casting, a frequency in the range from 0.5 to 5 MHz shall be used. The background noise shall not exceed 25 % of the distance amplitude correction curve (DAC). Transducers shall be utilized at their rated frequencies.

4.2.2 *Dual Element*, 5 MHz,  $\frac{1}{2}$  by 1 in. [13 by 25 mm], 12° included angle search units are recommended for sections 1 in. [25 mm] and under.

4.2.3 Other frequencies and sizes of search units may be used for evaluating and pinpointing indications.


#### 4.3 Reference Blocks:

4.3.1 Reference blocks containing flat-bottom holes shall be used to establish test sensitivity in accordance with 8.2.

4.3.2 Reference blocks shall be made from cast steels that give an acoustic response similar to the castings being examined.

4.3.3 The design of reference blocks shall be in accordance with Fig. 1, and the basic set shall consist of those blocks listed in Table 1. When section thicknesses over 15 in. [380 mm] are to be inspected, an additional block of the maximum test thickness shall be made to supplement the basic set.

4.3.4 Machined blocks with  $\frac{3}{32}$  in. [2.4 mm] diameter flat-bottom holes at depths from the entry surface of  $\frac{1}{8}$  in. [3 mm],  $\frac{1}{2}$  in. [13 mm], or  $\frac{1}{2}t$  and  $\frac{3}{4}$  in. [19 mm], or  $\frac{3}{4}t$  (where  $t$  = thickness of the block) shall be used to establish the DAC for the dual element search units (see Fig. 2).

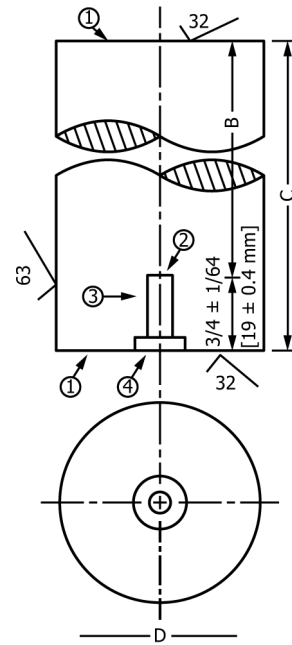

NOTE 1—Opposite ends of reference block shall be flat and parallel within 0.001 in. [0.025 mm].

NOTE 2—Bottom of flat-bottom hole shall be flat within 0.002 in. [0.051 mm] and the finished diameter shall be  $\frac{1}{4} + 0.002$  in. [6.4 + 0.050].

NOTE 3—Hole shall be straight and perpendicular to entry surface within 0°, 30 min and located within  $\frac{1}{32}$  in. [0.80 mm] of longitudinal axis.

NOTE 4—Counter bore shall be  $\frac{1}{2}$  in. [15.0 mm] diameter by  $\frac{1}{8}$  in. [3 mm] deep.

**FIG. 1 Ultrasonic Standard Reference Block**

**TABLE 1 Dimensions and Identification of Reference Blocks in the Basic Set (See Fig. 1)**

| Hole Diameter in $\frac{1}{64}$ ths, in. [mm] | Metal Distance (B), in. <sup>A</sup> [mm] | Overall Length (C), in. [mm] | Width or Diameter (D), min, in. [mm] | Block Identification Number |
|-----------------------------------------------|-------------------------------------------|------------------------------|--------------------------------------|-----------------------------|
| 16 [6.4]                                      | 1 [25]                                    | 1 $\frac{3}{4}$ [45]         | 2 [50]                               | 16-0100                     |
| 16 [6.4]                                      | 2 [50]                                    | 2 $\frac{3}{4}$ [70]         | 2 [50]                               | 16-0200                     |
| 16 [6.4]                                      | 3 [75]                                    | 3 $\frac{3}{4}$ [95]         | 2 [50]                               | 16-0300                     |
| 16 [6.4]                                      | 6 [150]                                   | 6 $\frac{3}{4}$ [170]        | 3 [75]                               | 16-0600                     |
| 16 [6.4]                                      | 10 [255]                                  | 10 $\frac{3}{4}$ [275]       | 4 [100]                              | 16-1000                     |
| 16 [6.4]                                      | B                                         | B + $\frac{3}{4}$ [B + 20]   | 5 [125]                              | 16-B00 <sup>B</sup>         |

<sup>A</sup> Tolerance  $\pm \frac{1}{8}$  in. [3 mm].

<sup>B</sup> Additional supplemental blocks for testing thickness greater than 10 in. [250 mm], see 4.3.3.

4.3.5 Each reference block shall be permanently identified along the side of the block indicating the material and the block identification.

4.4 *Couplant*—A suitable couplant having good wetting characteristics shall be used between the search unit and examination surface. The same couplant shall be used for calibrations and examinations.

### 5. Personnel Requirements

5.1 Personnel performing ultrasonic examination in accordance with this practice shall be qualified and certified in